





Toroidal transformer type 5N966

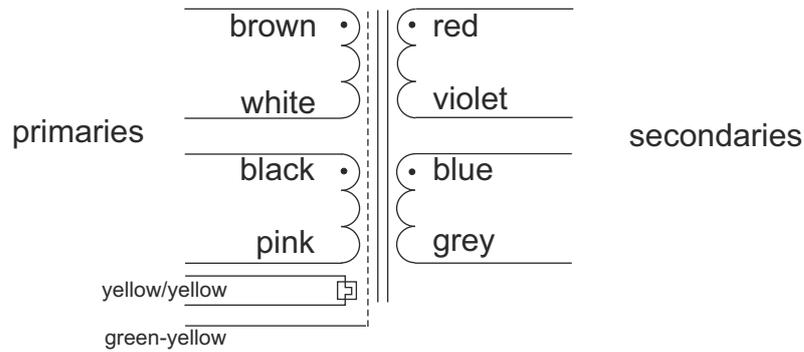


primaries in parallel for 115V input





secondaries in parallel for 115V output

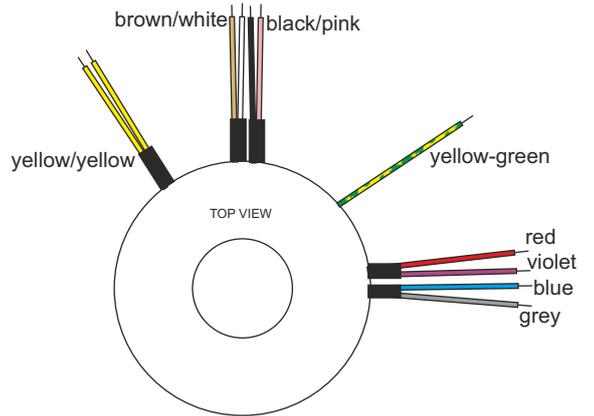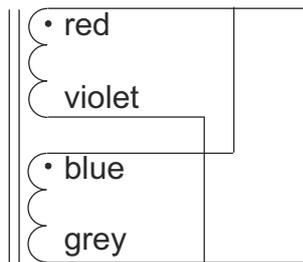

primaries in series for 230V input



secondaries in series for 230V output

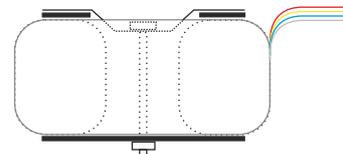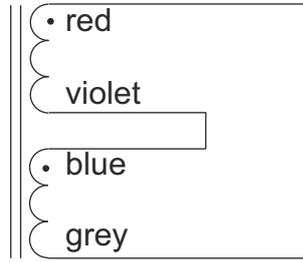

primaries: 2x 115V
 secondaries: 2x115V 0.57A
 total power rating: 130VA
 regulation:11%
 maximum leakage current: 0.06mA

Diameter 110mm
 Height 45mm
 Weight 1.8kg
 Height and weight are measured without mounting materials
 All leads are solid and approx 200mm long

Supplied mounting materials:
 1 metal washer Ø9cm
 2 neoprene washers Ø9cm
 1 bolt M5x50 with nut

With KEMA KEUR, ENEC, CE and UL/CSA approvals
 KEMA certificate 2159403.02 (KEMA label refers to EN61558 approval), UL filenumber E320377
 Built en tested according to EN60601-1

Built-in selfresetting thermal cutout to be switched in series with all primaries.

Static tapescreen between primary and secondary winding (green-yellow striped flexible wire to be connected to earth potential)

Time lag fuses to be used.
 for 230V primary: 0.63A 5x20mm,IEC127, high I²t value
 for 115V primary: 1.25A 5x20mm,IEC127, high I²t value

Secondary: none



Industrieweg 14
 NL-7161BX NEEDE
 The Netherlands
 P O - B o x 2 7
 NL-7160AA NEEDE
 The Netherlands
 Tel.+31 (0)545 263456
 Fax+31 (0)545 283457
 info@amplimo.nl
 http://www.amplimo.nl

HB	May 2003
©	Copyright Amplimo BV

5N966
 toroidal power transformer
 for medical purposes